

Instructions for Use

Connecting the Male Luer Valve

Single Use Only. Do not reprocess or reuse.
Not made with natural rubber latex.

Cat. No. : 251001001, 251001061



Cautions:

- Carefully follow the directions below to maintain the valve integrity.
- Only use standard Luer connection devices; non-standard syringes or connectors can damage the valve.
- A standard Luer connection must conform to the harmonized standards, ISO 594-1 and/or ISO 594-2. Syringes and female Luer connectors have a large variety of configurations and can vary significantly in design and dimensions.
- **DO NOT OVER-TIGHTEN** connections. **DO NOT USE** any instruments to tighten connections.

1. Using aseptic technique, remove the sterile device from the package. Discard if packaging is not intact.
2. Carefully connect by pushing the Male Luer Valve straight into the Luer connection using a clockwise, twisting motion.

DO NOT try to insert at an angle
See illustration 1 (a and b)

Male Luer Valve (MLV)

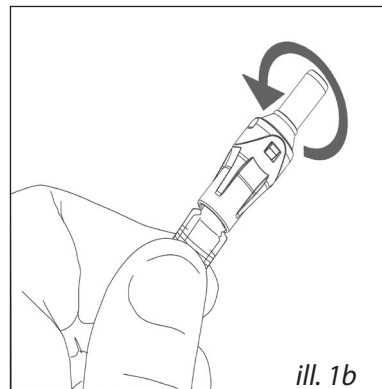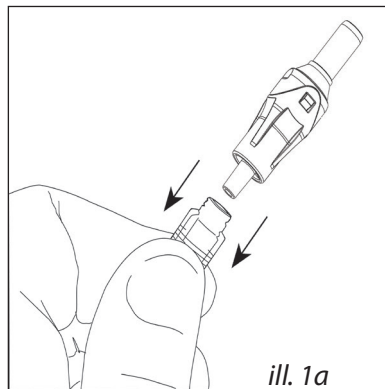

3. Twist counterclockwise to disconnect. The Male Luer Valve completely closes after each use and therefore does not require a separate cap.
4. Change device per facility protocol.
5. Dispose of used device per facility protocol for biocontaminated materials.

All HR® Medical Components are shipped bulk, non-sterile and are single patient use medical device components requiring further processing (e.g. assembly, packaging, sterilization) before clinical use. The buyer is responsible for determining effects of processing/multiple usage on these components, appropriateness of the component in the final application, and pre/post shelf life.

Halkey-Roberts®

2700 Halkey-Roberts Pl. N.
St. Petersburg, FL 33716 USA
727.471.4200
www.halkeyroberts.com
sales@halkeyroberts.com

US Patents 6,089,541 ~ 6,651,956 ~ 9,717,897
and other US and foreign patents issued and
pending Made in the USA